


Iao Deep Monitor Well, Maui (6-5230-002)
Fluctuations in the Water Table, Top of Transition Zone (TTZ), and Midpoint of Transition Zone (MPTZ)
From May 2006 through March 2025

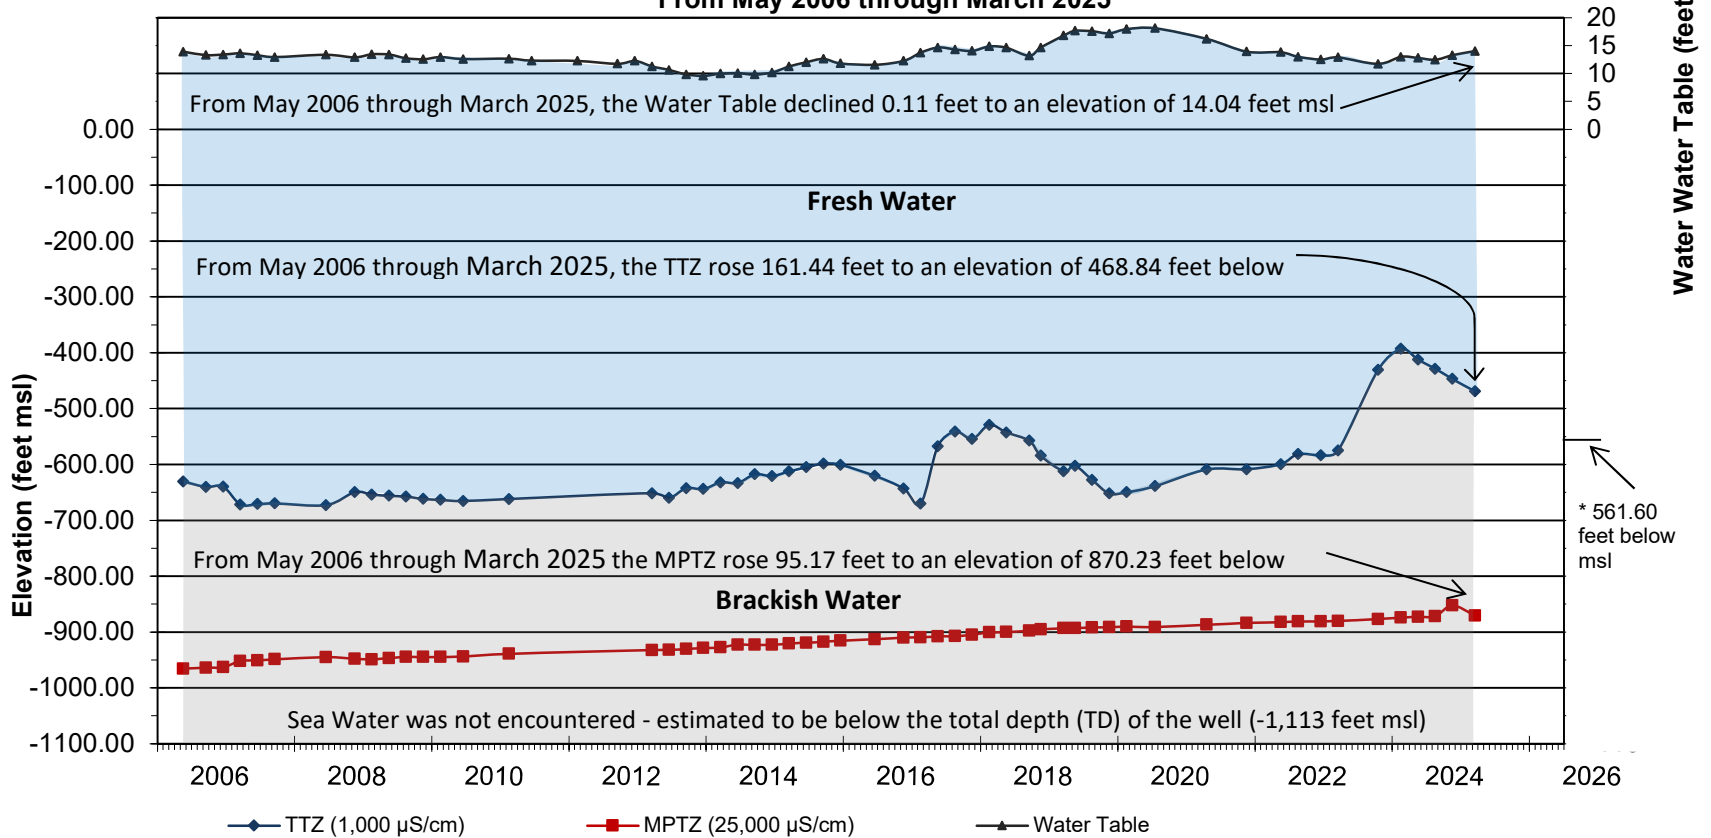

Notes: : (1) TTZ = 1,000 $\mu\text{S}/\text{cm}$ (~ 220 mg/L Cl^-); MPTZ = 25,000 $\mu\text{S}/\text{cm}$ (~ 8,500 mg/L Cl^-) (2) Fresh Water < 220 mg/L Cl^- , Brackish Water 220 mg/L Cl^- to 19,399 mg/L Cl^- , Sea Water >= 19,400 mg/L Cl^- ; (3) OS 421/425 = Ocean Sensors CTD (absolute conductivity); (4) RBR 12895 = RBR Global CTD (Specific Conductivity); (5) msl = mean sea level.

* Since the year 2006, the MPTZ rose 95.17 feet, below a calculated Ghyben-Herzberg equilibrium elevation of approximately 561.60 feet below msl, relative to the Water Table measured at 14.04 feet above msl.